

Sample Received: February 9, 2026

COA Issued: February 12, 2026

PRODUCT INFORMATION

Vendor:
BioSync Solutions

Sample Name:
Sermorelin 10mg

Sample Type:
White lyophilized powder

Batch Number:
26085

MW
3357.77 g/mol

ANALYTICAL METHODS

Identity: Confirmed via MALDI—MS

Purity: RP-HPLC (214 nm)



Content: HPLC quantitation

TEST RESULTS


Specification	Result	Method	
Identity: Sermorelin	Sermorelin	MALDI-MS	✓ Conforms
Content	11.05 mg	HPLC Quantitation	✓ Conforms
Overall Purity	99.7%	RP-HPLC (214 nm)	✓ Conforms

ANALYTICAL DATA

HPLC Chromatogram (Retention Time: 2.342 min)

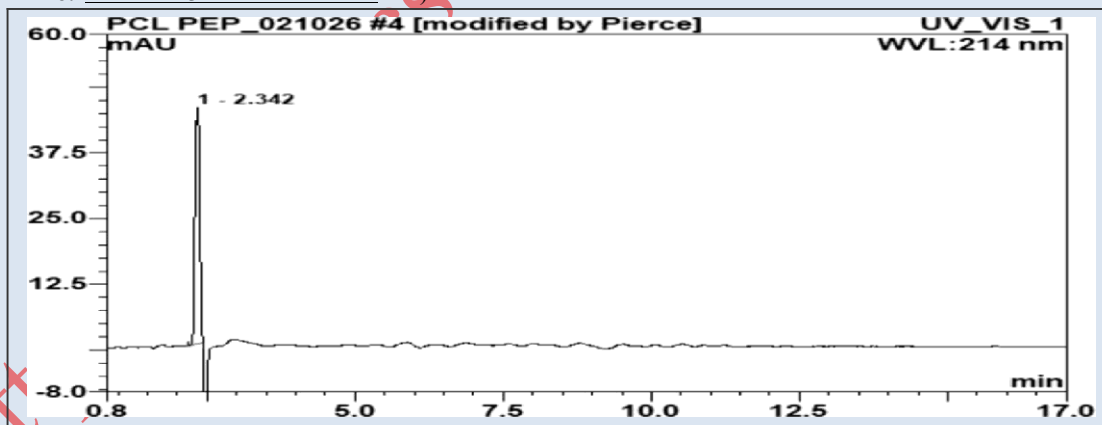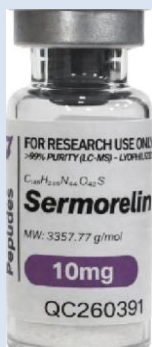

Mass Spectrum (MALDI-MS)

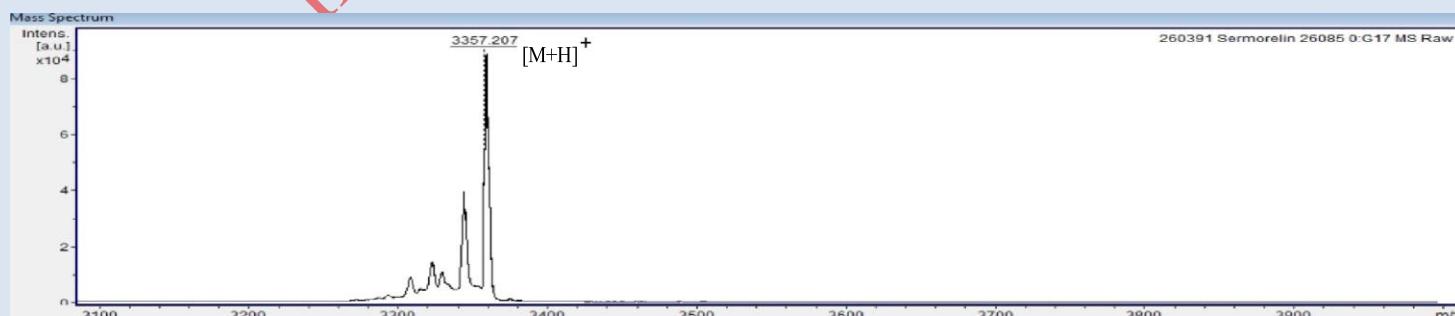

This Certificate of Analysis certifies that the above-referenced sample was tested according to Bio Gen Lab's standard operating procedures. All results reported herein are accurate and complete to the best of our knowledge. This document is intended solely for the use of the addressee and may contain confidential information. Visit: <https://biogenlab.org>.

Shane Straight

Shane Straight, M.S.

Principal Chemist, Bio Gen Labs